





B2CBH-02

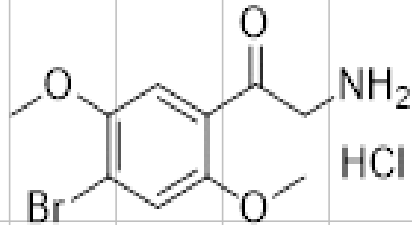

Parameters		
	Parameter	Value
1	Title	Sep25-2020.260.1.1r
2	Origin	Bruker BioSpin GmbH
3	Instrument	spect
4	Solvent	
5	Temperature	
6	Pulse Sequence	zg30
7	Number of Scans	16
8	Receiver Gain	406.0
9	Relaxation Delay	1.0000
10	Pulse Width	15.0000
11	Acquisition Date	2020-09-25T16:47:50
12	Spectrometer Frequency	400.13
13	Spectral Width	8223.7
14	Lowest Frequency	-1313.8
15	Nucleus	¹ H

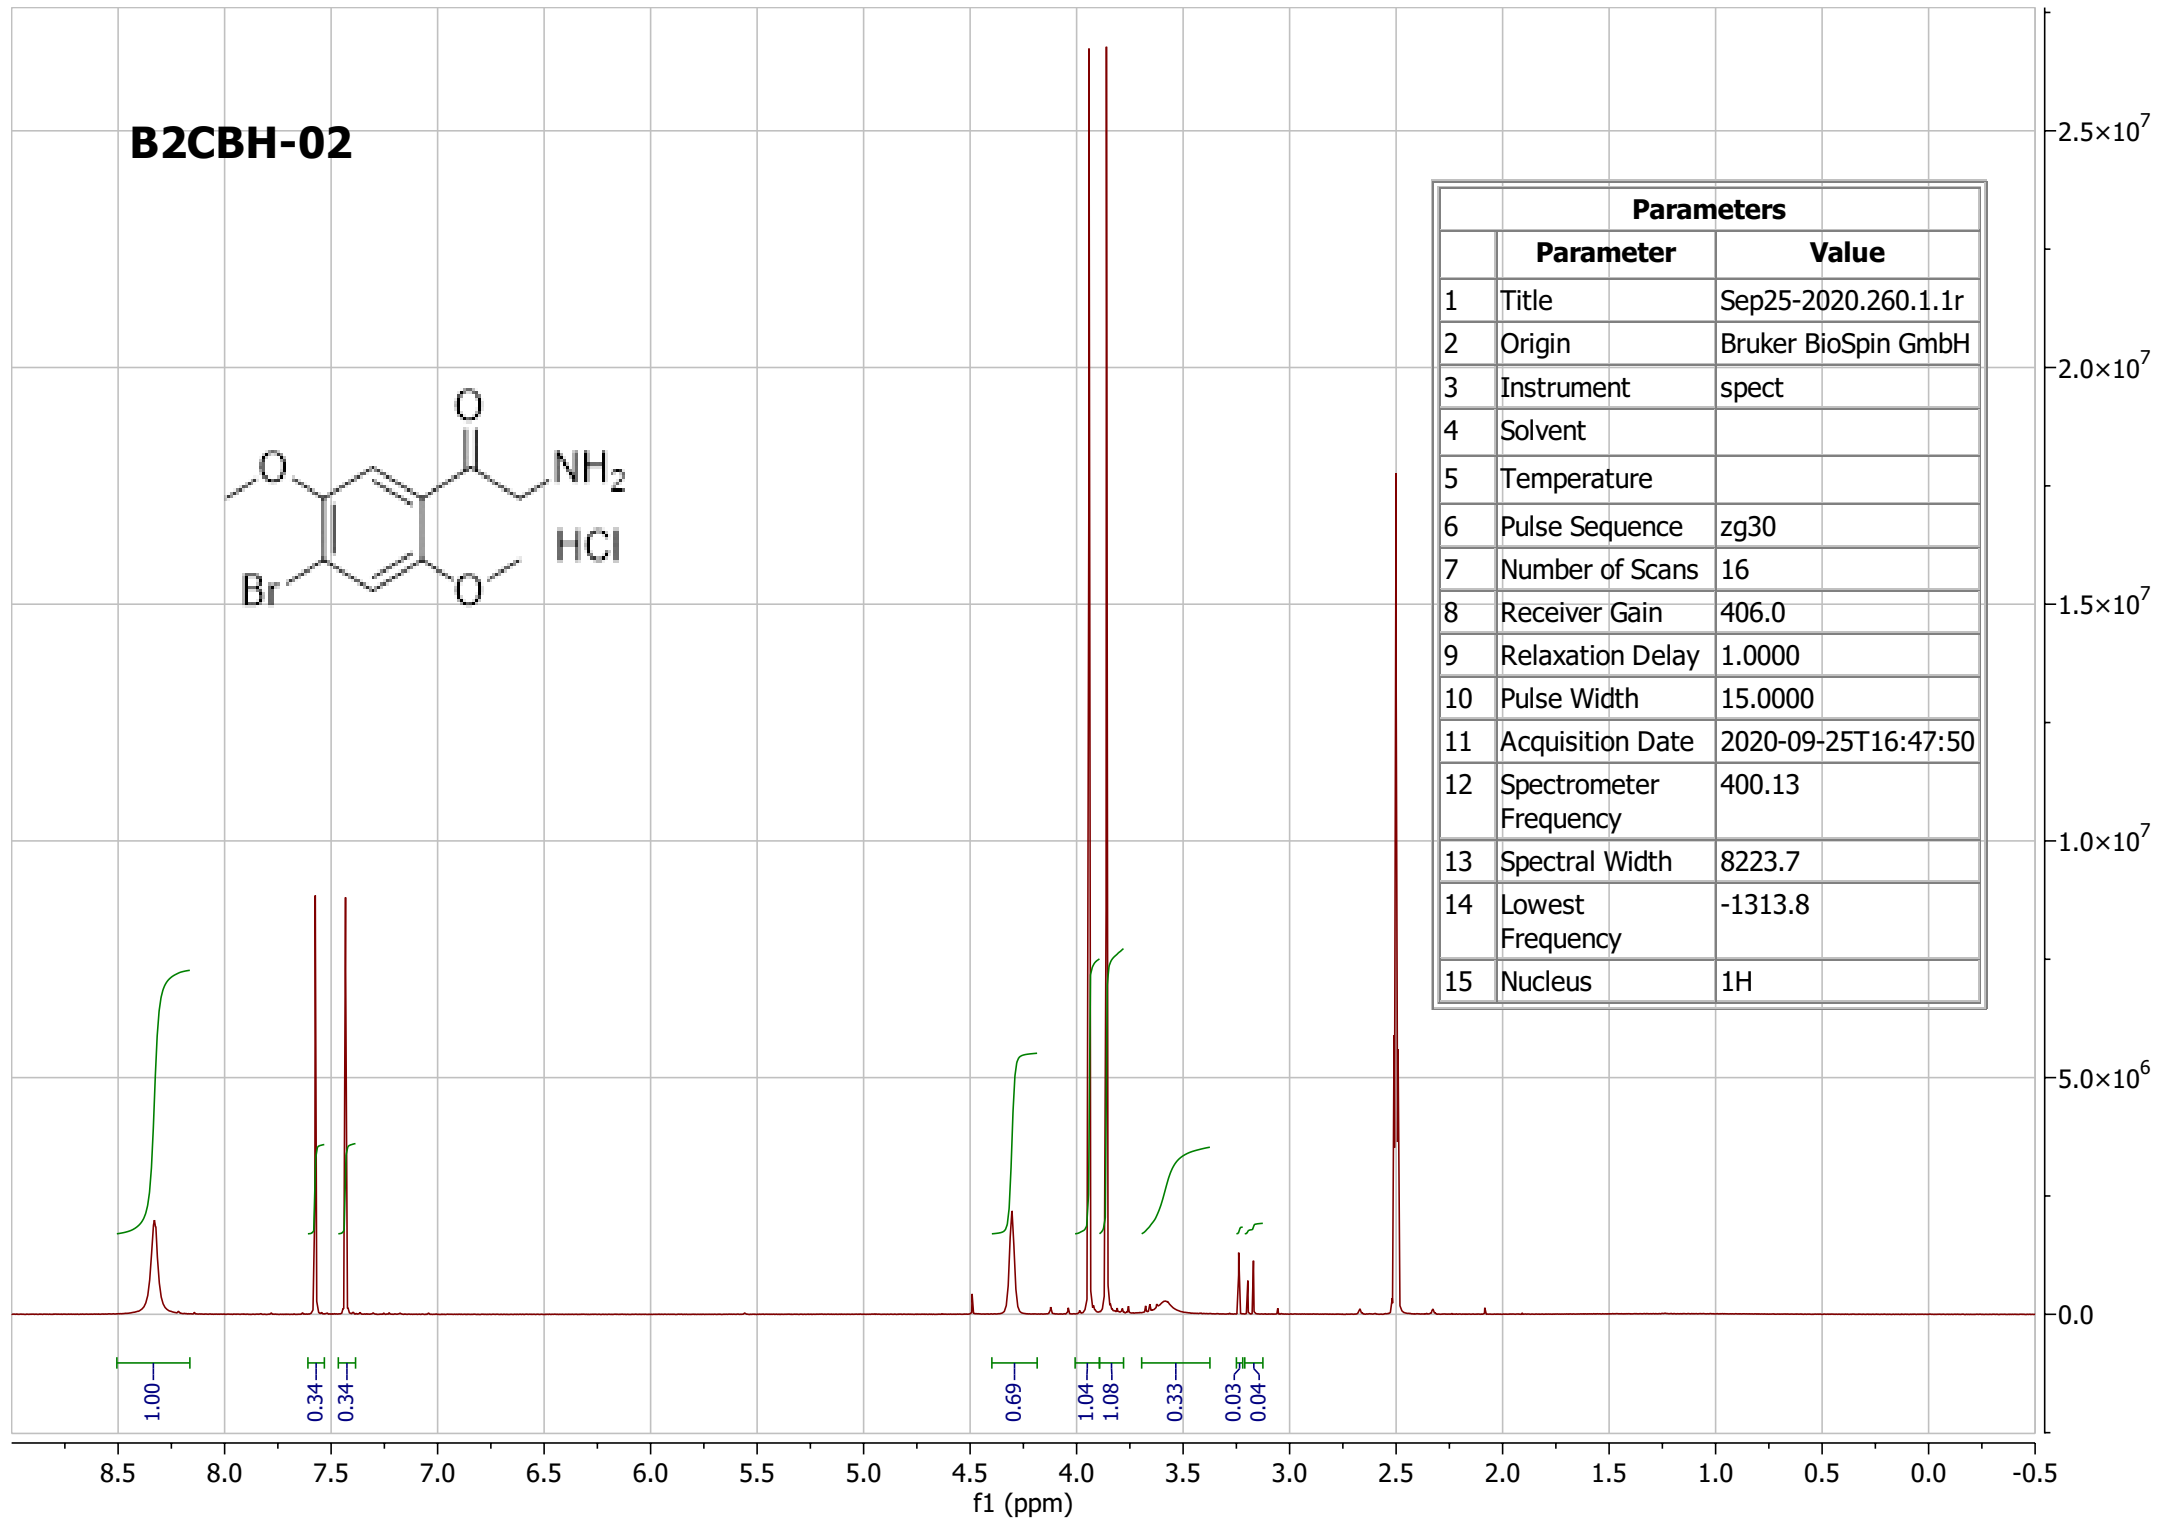

B2CBH-02

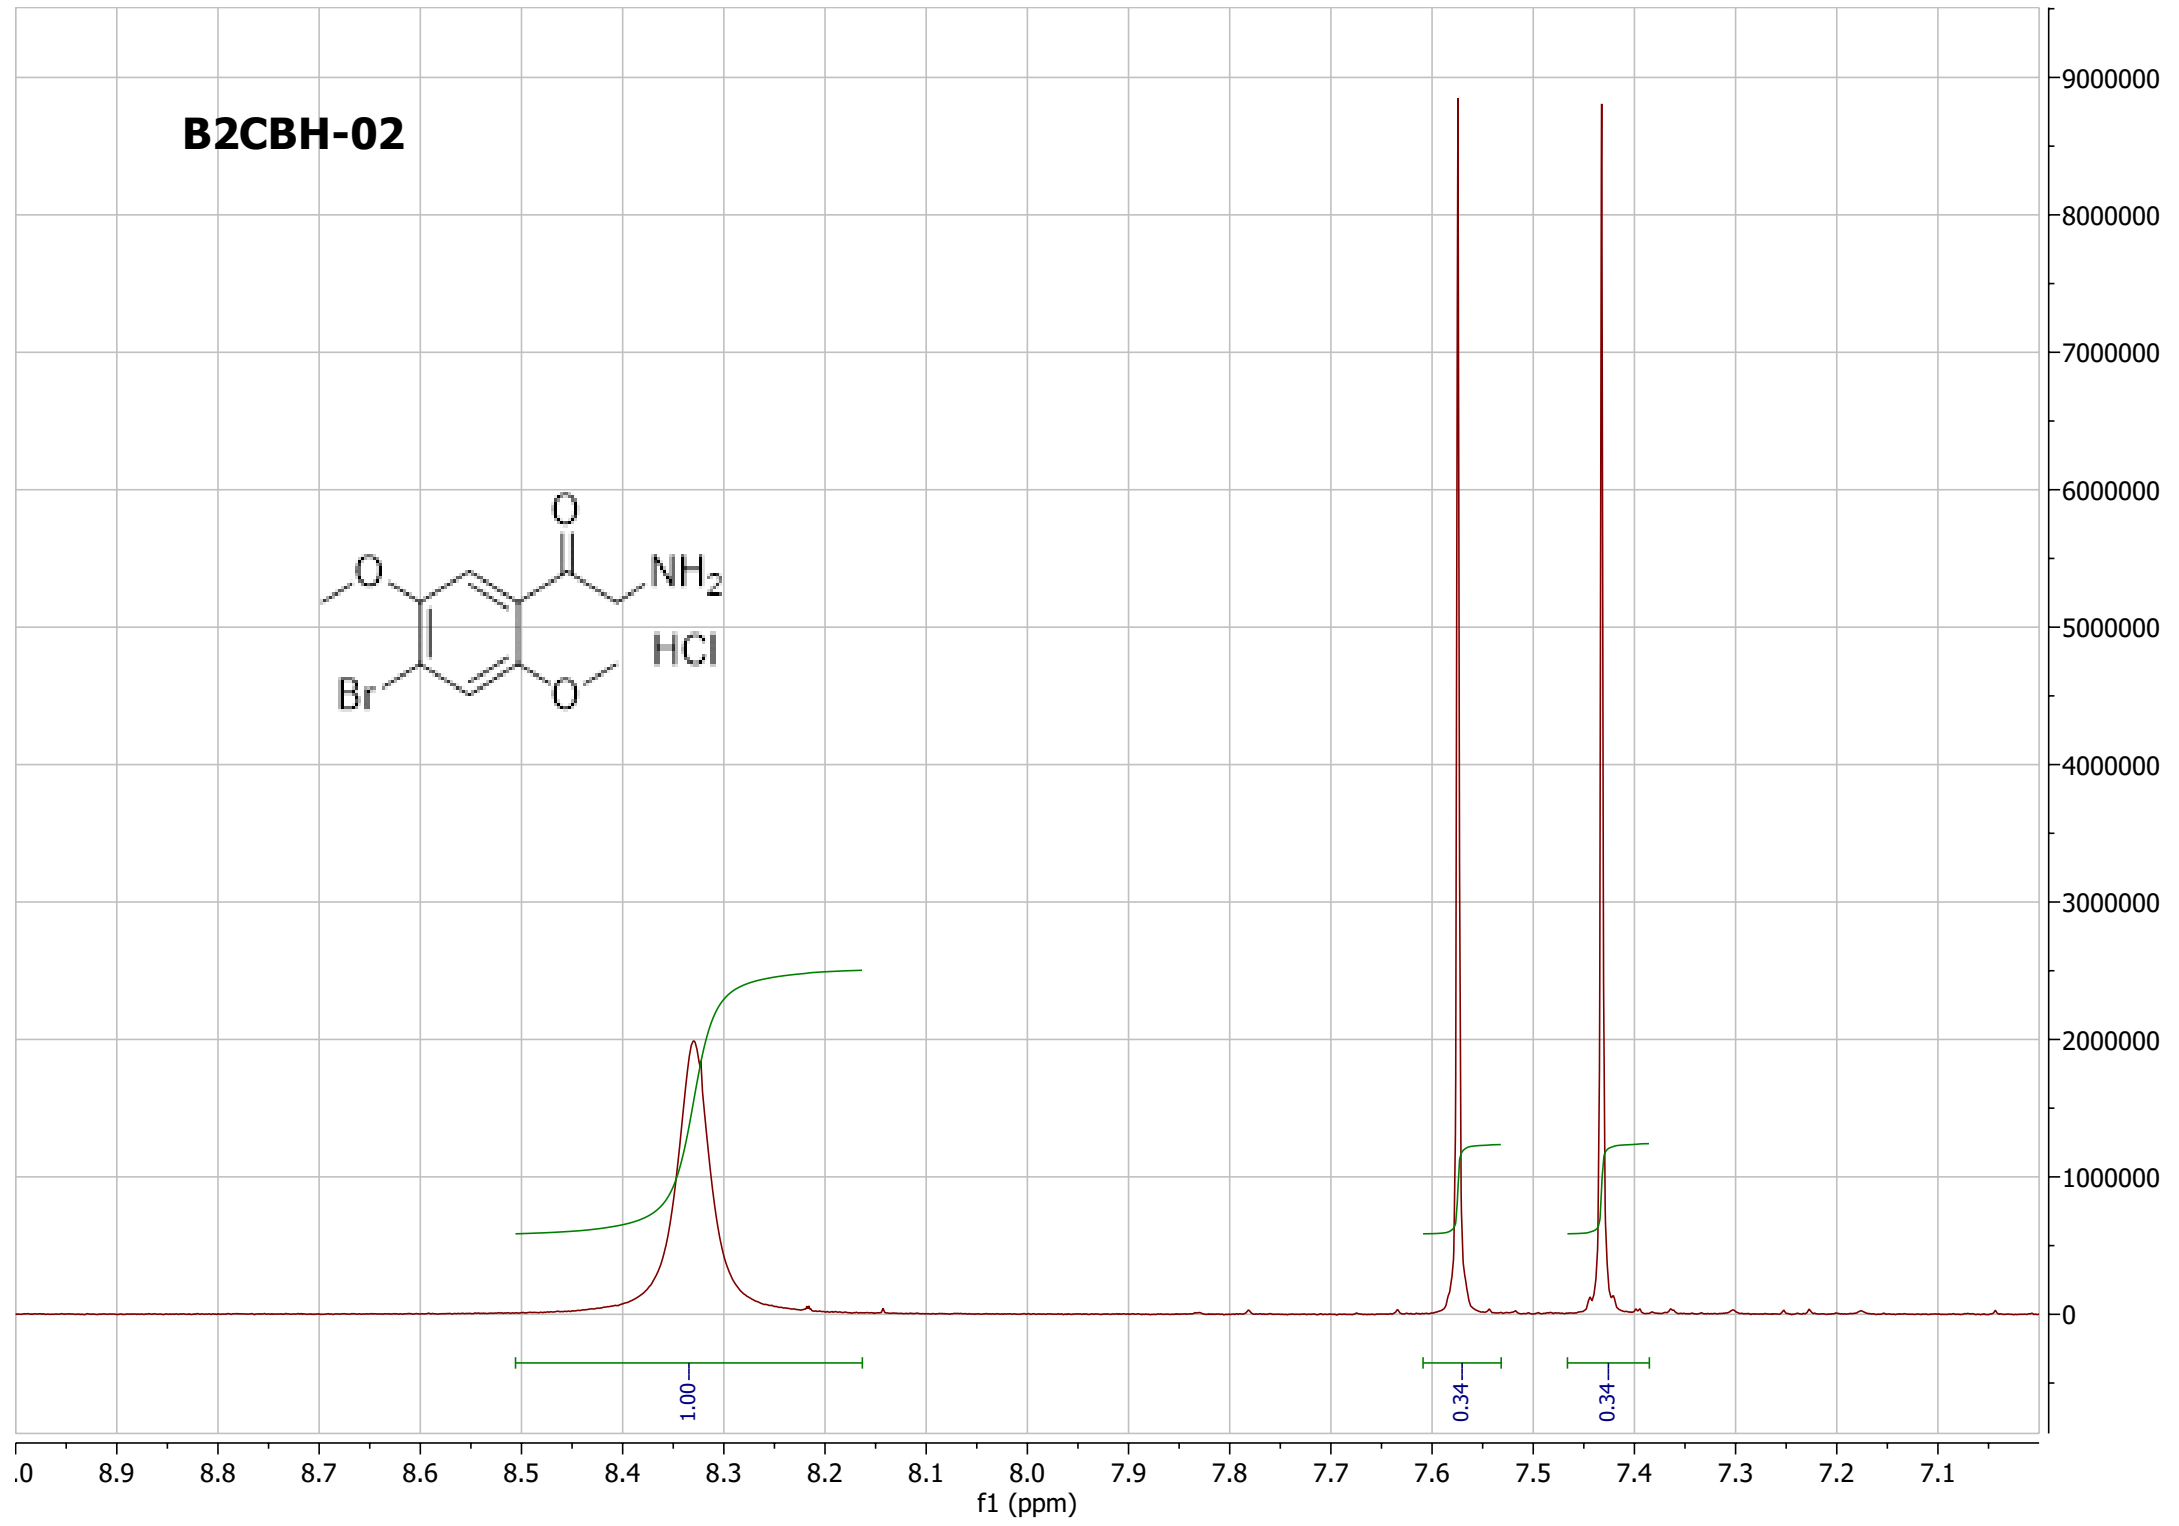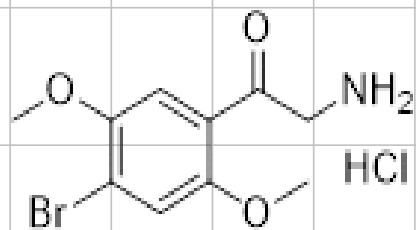

B2CBH-02

